



CENTRAL
— P E P T I D E S —

support@centralpeptides.ca

centralpeptides.ca


Certificate of Analysis

Semax 10 mg

Multi-Agonist Peptide

Compound	: Semax	Client	: Internal Use
Lot (Batch) Number	: CP-SE-0927	Website	: centralpeptides.ca
Analysis Date	: 2026-01-18		
Purity %	: 99.60%		
Quantity	: 10.56 mg		
Method	: HPLC-UV-MS		

High Performance Liquid Chromatography (HPLC) UV – Purity Test

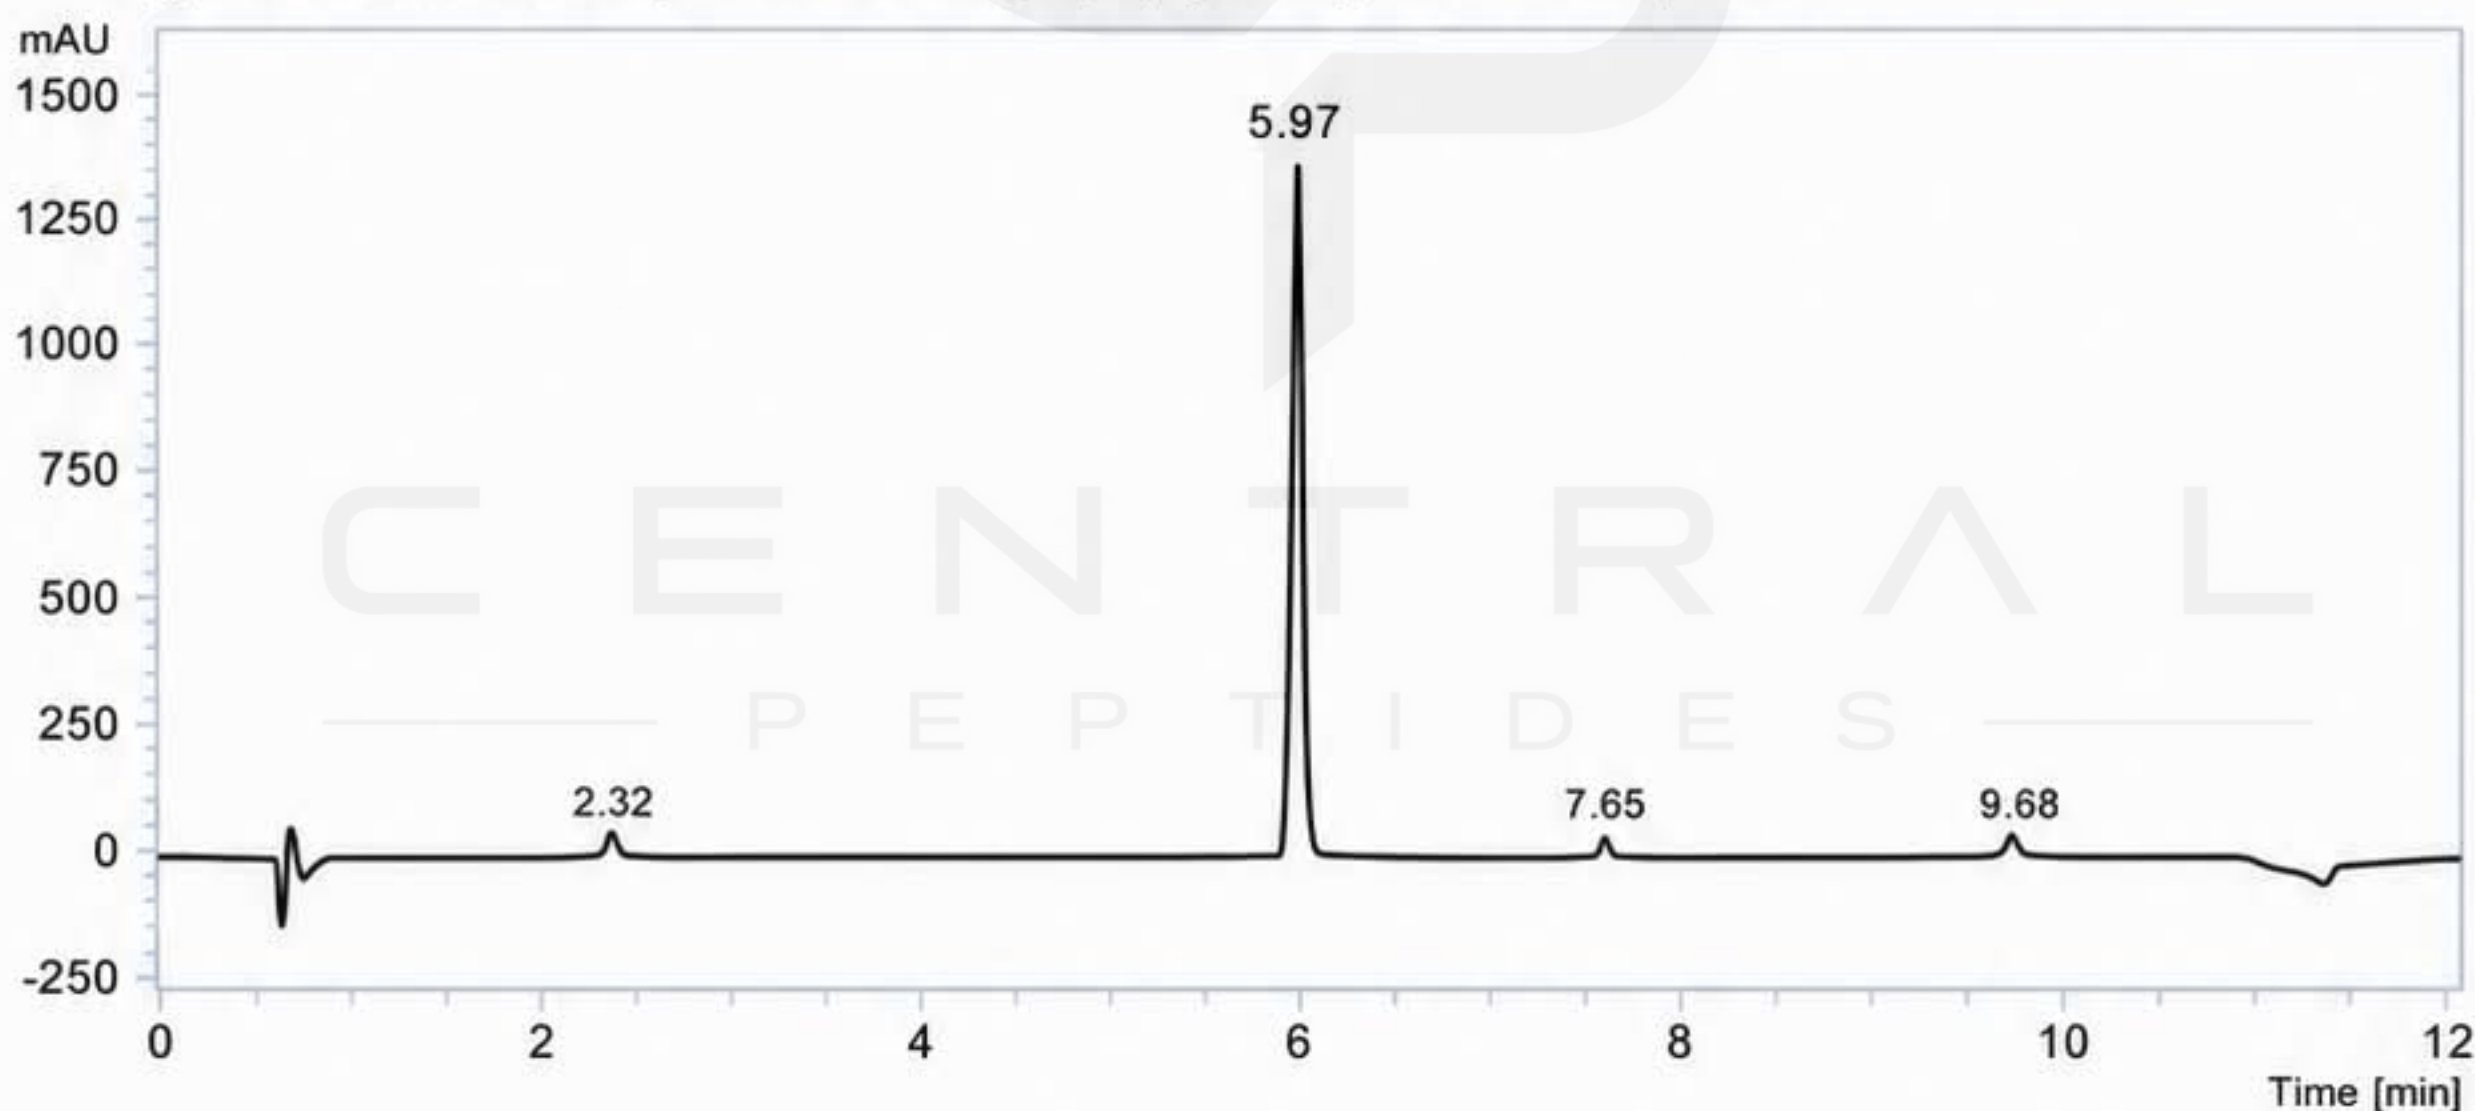

CP-SE-0927 [modified by User]

UV_VIS_1 WVL:220 nm

PEAK LIST

Peak	Time (min)	Area	%Area	Amount (mg)	Identity
1	2.32	4.98E+04	0.19	0.0201 mg	Impurity
2	5.97	2.59E+07	99.60	10.5600 mg	Semax
3	7.65	6.62E+04	0.25	0.0264 mg	Impurity
4	9.68	2.45E+04	0.09	0.0093 mg	Impurity

Analysis Performed by
Central Peptides
Analytical Chemist
Central Peptides
support@centralpeptides.ca

Loic Becham

Note: Injectable peptides may contain salts and sugars to aid in solubility and act as pH buffers.

These are not normally detected using UV and are not considered impurities.

2026-01-18